

Evaluation of the effectiveness of X-ray protective aprons in experimental and practical fields

著者	Mori Hiroshige, Koshida Kichiro, Ishigamori Osamu, Matsubara Kosuke
journal or publication title	Radiological Physics and Technology
volume	7
number	1
page range	158-166
year	2014-01-01
URL	http://hdl.handle.net/2297/39049

doi: 10.1007/s12194-013-0246-x

Hiroshige Mori^{1,2,*} · Kichiro Koshida³ · Osamu Ishigamori¹ · Kosuke Matsubara³

Evaluation of the effectiveness of X-ray protective aprons in experimental and practical fields

Author-affiliation information:

¹Department of Radiology, Hokkaido Social Insurance Hospital,

1-8-3-18 Nakanoshima, Toyohira, Sapporo, Hokkaido 062-8618, Japan

²Department of Quantum Medical Technology, Division of Health Sciences, Graduate School of Medical Science, Kanazawa University,

5-11-80 Kodatsuno, Kanazawa, Ishikawa 920-0942, Japan

³School of Health Sciences, College of Medical, Pharmaceutical and Health Sciences, Kanazawa University, 5-11-80 Kodatsuno, Kanazawa, Ishikawa 920-0942, Japan

*Corresponding author details:

Hiroshige Mori

Department of Radiology, Hokkaido Social Insurance Hospital,

1-8-3-18 Nakanoshima, Toyohira, Sapporo, Hokkaido 062-8618, Japan

Tel: +81-11-831-5151

Fax: +81-11-821-3851

E-mail: 8598fbjq@jcom.home.ne.jp

1 Abstract

2 Few practical evaluation studies have been conducted on X-ray protective aprons in
3 workplaces. We examined the effects of exchanging the protective apron type with
4 regard to exposure reduction in experimental and practical fields, and discuss the
5 effectiveness of X-ray protective aprons. Experimental field evaluations were performed
6 by measurement of the X-ray transmission rates of protective aprons. Practical field
7 evaluations were performed by estimation of the differences in the transit doses before
8 and after the apron exchange. An 0.50-mm lead-equivalent-thick non-lead apron had the
9 lowest transmission rate among the 7 protective aprons, but weighed 10.9 kg and was
10 too heavy. The 0.25-mm and 0.35-mm lead-equivalent-thick non-lead aprons differed
11 little in the practical field of interventional radiology. The 0.35-mm lead apron had
12 lower X-ray transmission rates and transit doses than the 0.25-mm lead-equivalent-thick
13 non-lead apron did, and each of these differences exceeded 8% in the experimental field
14 and approximately 0.15 mSv/month in the practical field of computed tomography ($p <$
15 0.01). Therefore, we concluded that the 0.25-mm lead-equivalent-thick aprons and
16 0.35-mm lead apron are effective for interventional radiology operators and computed
17 tomography nurses, respectively.

18

19

20 Keywords:

21 analysis of covariance, computed tomography, interventional radiology, protective
22 apron, radiation protection, X-ray transmission rates

23

1 1. Introduction

2 Recently, attention has focused on orthopedic injuries attributed to the weight of
3 X-ray protective aprons [1-3]. To resolve this problem, lighter aprons, made of
4 composite materials, have been developed successfully [4-6]. These composite
5 materials include several heavy metals such as copper, yttrium, tin, antimony, barium,
6 tungsten, and lead [7-9]. However, manufacturers have not adequately released
7 information about these composites [9-11].

8 The figures of merit of these protective aprons are commonly expressed as
9 lead-equivalent thicknesses, which are measured only for specific X-ray energies [10,
10 11]. However, various energies are used in workplaces [9, 10]. There is also a difference
11 in X-ray attenuation between pure lead and composite materials, which is determined by
12 X-ray energies [9]. Therefore, the X-ray transmission rates of protective aprons, which
13 are often measured at optional energies, differ among manufacturers, despite having the
14 same lead-equivalent thicknesses [10, 11].

15 Differences in lead-equivalent thicknesses or X-ray transmission rates among
16 protective aprons are not always reflected in the radiation fields of workplaces: practical
17 fields. For example, in interventional cardiology, no significant difference in X-ray
18 shielding performance was reported between 0.25-mm and 0.35-mm
19 lead-equivalent-thick non-lead aprons [12]. However, there have been few practical
20 evaluation studies in workplaces [13].

21 Here, we evaluated the effects of personal exposure reduction in experimental and
22 practical fields upon exchanging the X-ray protective apron type worn by medical staff.
23 The experimental field evaluation was performed by measurement of the X-ray
24 transmission rates of protective aprons. The practical field evaluation was performed by

1 estimation of the differences in the transit doses before and after the apron exchange,
2 with the values measured by individual monitoring. Thus, we aim to discuss the
3 effectiveness of X-ray protective aprons.

4 5 6 2. Materials and methods

7 We researched the effects of exposure reduction before and after the exchange of the
8 X-ray protective apron types as follows:

- 9 a) Exchanging 0.25-mm lead-equivalent-thick non-lead aprons for 0.35-mm
10 lead-equivalent-thick non-lead aprons, for the first and second abdominal
11 interventional radiology (IVR) operators
- 12 b) Exchanging 0.25-mm lead aprons for 0.50-mm lead-equivalent-thick non-lead
13 aprons, for interventional cardiology operators
- 14 c) Exchanging 0.25-mm lead-equivalent-thick non-lead aprons for 0.35-mm lead
15 aprons, for nurses in a workplace where computed tomography (CT) is performed

16 Table 1 shows the specifications and use conditions of the X-ray protective aprons.

17 We tested the statistical differences in X-ray transmission rates and transit doses
18 before and after the apron exchange in the above cases. If there were statistical
19 differences, we computed the statistical estimated differences. We compared the
20 statistical results of these X-ray transmission rates and transit doses.

21 22 2-1. Figures of merit of the X-ray protective aprons

23 We measured the lead-equivalent thicknesses of the X-ray protective aprons as
24 figures of merit. Currently, there are various lead-equivalent thickness evaluation

Table 1

1 methods [10, 11, 14]. We adopted a computational method from an apron attenuation
2 formula [14] because it is possible to re-inspect lead-equivalent thicknesses easily in all
3 facilities with only aluminum filters, which are easier to acquire than lead filters.

4 First, with aluminum filters, we measured the half-value layer of the primary X-rays
5 and computed their effective energy. Second, we computed the lead attenuation
6 coefficient, μ_{pb} , from the effective energy of the primary X-rays [15], considering that
7 the attenuation coefficient is a function of photon energy. Third, we measured the doses
8 through and without protective aprons, I' and I . Last, we calculated the apron's
9 lead-equivalent thickness, d_{apron} , by substituting μ_{pb} , I' and I for the following apron
10 attenuation formula:

$$11 \quad I' = I \cdot e^{-\mu_{\text{pb}} \cdot d_{\text{apron}}}, \quad (1)$$

$$12 \quad d_{\text{apron}} = -\frac{1}{\mu_{\text{pb}}} \cdot \ln \frac{I'}{I}. \quad (2)$$

13 The medical X-ray apparatus used in this study was a DRX-3724HD X-ray tube with
14 KXO-80G inverter-type high-potential generators (Toshiba Medical Systems, Tochigi,
15 Japan), with an inherent filtration of 1.1-mm aluminum-equivalent thickness and an
16 additional filtration of 2.7-mm aluminum-equivalent thickness. An ionization chamber,
17 the DC300 3-cc thimble reference chamber (Wellhöfer, Schwarzenbruck, Germany),
18 was interfaced with a RAMREC1500B dosimeter (Toyomedic, Tokyo, Japan). A
19 2.8-cm-diameter lead collimator was used for narrowing the X-ray beam. Figure 1
20 shows the geometries of these materials and the X-ray protective aprons. Aluminium
21 filters with a fineness of 99.99% for measuring the half-value layer were set at a 30-cm
22 distance from the focal spot of an X-ray tube.

23 Primary X-rays were generated at 250 mA, 50 ms, and 120 kVp. In addition, for

Fig. 1

1 adjusting the effective energy of the primary X-rays to approximately 60 keV [14], an
2 additional filter comprising 2.0-mm aluminum-equivalent and 0.2-mm
3 copper-equivalent thicknesses was set at a 30-cm distance from the focal spot of an
4 X-ray tube.

5

6 2-2. Experimental field evaluation of X-ray protective aprons

7 2-2-1. Effective energy of primary X-rays used in an experimental field

8 We computed the effective energy of the primary X-rays used in an experimental
9 field by measuring the half-value layer of the medical X-ray apparatus.

10 The half-value layer measurement of the primary X-rays was performed with the
11 same materials as in section 2-1, although the additional aluminum–copper filter was
12 not used. The aluminum filter geometry for measurement of the half-value layer, a lead
13 collimator to narrow the X-ray beam, and an ionization chamber were set at distances of
14 30 cm, 55 cm, and 180 cm, respectively, from the focal spot of an X-ray tube.

15 Primary X-rays were generated at 200 mA and 36 ms. We measured the half-value
16 layers of the primary X-rays at 5 tube potentials: 50 kVp, 60 kVp, 80 kVp, 100 kVp,
17 and 120 kVp. The effective energy of the primary X-rays was computed from the
18 measured half-value layers [15].

19

20 2-2-2. X-ray transmission rates of protective aprons in an experimental field

21 The X-ray transmission rate of a protective apron, T , is an index that estimates the
22 effect of exposure reduction in a practical field, and is given as follows:

23
$$T = \frac{I'}{I} \cdot 100. (3)$$

1 There are two measurement methods for the X-ray transmission rate with the narrow
2 primary X-ray beam or the broad scatter X-ray beam [11, 16]. In this study, we adopted
3 the narrow primary X-ray beam because the used ionization chamber volume was too
4 small to use the broad scatter X-ray beam.

5 We measured the X-ray transmission rates of the X-ray protective aprons with the
6 above formula (3) and the narrow beam. X-ray transmission rate measurements were
7 performed with the materials and geometry (Fig. 1) of section 2-1, although filters were
8 not used. Primary X-rays used the same tube current and potentials as in section 2-2-1,
9 but the exposure time was 50 ms. We performed analysis of variance (ANOVA) to
10 compare the X-ray transmission rates between the protective aprons in case a), b), and
11 c) because of the two-way layout design with the five effective energies of primary
12 X-rays per apron. Microsoft Office Excel 2007 Service Pack 3 software was used
13 (Microsoft, Washington, U.S.A.). If there was a statistically significant difference by
14 ANOVA, we estimated the difference before and after apron exchange.

15

16 2-3. Practical field evaluation of X-ray protective aprons

17 2-3-1. Transit doses of X-ray protective aprons in a practical field

18 Medical staff occupational exposure was managed with personal dosimeter readings in
19 a practical field. The effect of the exposure reduction in an X-ray protective apron ought
20 to be reflected in the individual monitoring results. However, we could not merely
21 compare exposure doses before and after apron exchange, because the working hours
22 (i.e., the exposed doses to aprons) differed before and after apron exchange.
23 Accordingly, we adopted an analysis of covariance (ANCOVA) to evaluate the effect of
24 the X-ray protective apron exchange in a practical field.

1 ANCOVA is a general linear model-based statistical technique that has been presented
2 as an extension of regression analysis and ANOVA [17]. ANCOVA is used for
3 examining one-way layout design with the covariate as a nuisance factor. The covariate
4 is the extraneous variable that influences each level's quantitative variable at one factor.
5 Using the quantitative variable as a dependent variable, the regression line is given as
6 follows:

7
$$A_i: y_{ij} = \alpha_i + \beta_i x_{ij} \quad (j = 1, 2, 3, \dots, n_i), \quad (4)$$

8 where A_i is a level, called the qualitative independent variable, y_{ij} is the quantitative
9 variable, called a dependent variable, α_i is a constant term, β_i is the inclination, and
10 x_{ij} is the covariate, called a quantitative independent variable. α_i and β_i are not
11 simply calculated at the general linear model regression analysis, but are calculated
12 from the correlation of x_{ij} with y_{ij} , called a covariance [17, 18]. ANCOVA is
13 performed among quantitative variable levels with the residual error between the
14 observed dependent variable and the predicted dependent variable from formula (4).
15 Therefore, we can control the covariate-induced variance and increase the statistical
16 precision to detect the differences among levels at one factor.

17 In ANCOVA, there are 2 prerequisite conditions for which nothing is the significant
18 interaction between the qualitative and quantitative independent variables:

19
$$\beta_1 = \beta_2 = \beta_3 = \dots = \beta_n, \quad (5)$$

20 and there is a significant linear relationship between a quantitative independent variable
21 and a dependent variable:

22
$$\beta_i \neq 0 \quad (i = 1, 2, 3, \dots, n). \quad (6)$$

23 The statistical hypothesis (5) is not rejected by the F-test and is called a regressive

1 parallelism test. The statistical hypothesis against the alternative hypothesis (6) is
2 rejected by the F-test and is called a regressive significant test.

3 When ANCOVA was performed in this study, it was possible to remove the variance
4 of the exposed doses to aprons as a nuisance factor from the variance of the transit doses
5 through aprons, because exposed doses are covariates that influence transit doses.
6 Accordingly, we can compare the differences in the transit doses among several apron
7 types in a practical field without the influence of individual operation times before and
8 after apron exchange.

9 From individual monitoring results with personal dosimeters, we estimated the
10 difference in transit doses between the protective aprons in cases a), b) and c).
11 Individual monitoring was performed monthly with glass badges (Chiyoda Technol,
12 Tokyo, Japan). Personal dosimeters were worn at the collar level above the protective
13 apron and at the body level beneath the protective apron. The monthly measured collar
14 level value, $H_P(10)_{\text{collar/month}}$, and the monthly measured body level value,
15 $H_P(10)_{\text{body/month}}$, were shown as personal dose equivalents, defined in the
16 International Commission on Radiation Units and Measurements (ICRU) Report 51
17 [19] at a tissue depth of 10 mm. The examination period included 2 years before and 2
18 years after the apron exchange. To estimate the difference in transit doses between the
19 protective aprons, we performed ANCOVA as described above. $H_P(10)_{\text{body/month}}$, the
20 transit dose through the protective apron, was a quantitative variable.
21 $H_P(10)_{\text{collar/month}}$, the exposed dose to the protective apron, was a covariate. When the
22 X-ray protective apron type is expressed by 'A_i', formula (4) is updated as follows:

23
$$A_i: H_P(10)_{\text{body/month},ij} = \alpha_i + \beta_i \cdot H_P(10)_{\text{collar/month},ij} \quad (j = 1,2,3,\dots,12). \quad (7)$$

1 The significant difference of $H_P(10)_{\text{body/month}}$, after excluding covariates, is the
2 difference in the transit doses before and after apron exchange, $\Delta H_P(10)_{\text{body/month}}$:

3
$$\Delta H_P(10)_{\text{body/month}} = |\alpha_2 - \alpha_1|. \quad (8)$$

4 where α_1 and α_2 are constant terms before and after apron exchange, estimated by
5 formula (7). Microsoft Office Excel 2007 Service Pack 3 software was used (Microsoft,
6 Washington, U.S.A.).

7 In addition, if there were statistical differences in cases a), b), and c), we calculated
8 the decreased annual effective dose by using $\Delta H_P(10)_{\text{body/month}}$. The monthly
9 effective dose, $E_{\text{eff/month}}$, for inhomogeneous exposure is given as follows [20]:

10
$$E_{\text{eff/month}} = 0.11 \cdot H_P(10)_{\text{collar/month}} + 0.89 \cdot H_P(10)_{\text{body/month}}. \quad (9)$$

11 Because $H_P(10)_{\text{collar/month}}$ does not vary with apron exchange, the reduction in the
12 annual effective dose, $\Delta E_{\text{eff/year}}$, was obtained from the following equation:

13
$$\Delta E_{\text{eff/year}} = 12 \cdot 0.89 \cdot \Delta H_P(10)_{\text{body/month}}. \quad (10)$$

14

15 2-3-2. Dose reduction rate of protective aprons in a practical field

16 We performed a t-test of the dose reduction rates of X-ray protective aprons in a
17 practical field to re-inspect the ANCOVA results. The dose reduction rate of an X-ray
18 protective apron, r_{ik} , is given as follows:

19
$$r_{ik} = \frac{H_P(10)_{\text{body/month}}}{H_P(10)_{\text{collar/month}}} \cdot 100 \quad (k = 1, 2, 3, \dots, 12). \quad (11)$$

20 We compared the ANCOVA and this t-test result for cases a), b), and c).

21

22

1 3. Results

2 3-1. Figure of merit of the X-ray protective aprons

Table 2

3 Table 2 shows the measured lead-equivalent thicknesses of the X-ray protective
4 aprons. The lead-equivalent thicknesses of the 2 lead aprons were almost their nominal
5 thicknesses. However, the lead-equivalent thicknesses of the 5 non-lead aprons were
6 lower than expected. The effective energy used for these measurements was 62.5 keV.

7

8 3-2. Experimental field evaluation of X-ray protective aprons

Fig. 2

9 Figure 2 shows the relationship between the tube potential and the effective energy of
10 the primary X-rays in an experimental field. When the tube potential was varied from
11 50 kVp to 120 kVp, the effective energy of primary X-rays was varied from 31.4 keV to
12 49.3 keV.

Fig. 3

13 Figure 3 shows the relationship between effective energy and X-ray transmission
14 rates of protective aprons. The X-ray transmission rate increased along with the
15 effective energy. There were significant differences in X-ray transmission rates after
16 apron exchange in all section 2 cases ($p < 0.01$). There was also a synergistic effect
17 between effective energy and X-ray transmission rates of protective aprons in all section
18 2 cases ($p < 0.01$). The 0.50-mm lead-equivalent-thick non-lead apron had the lowest
19 transmission rate among the 7 protective aprons.

Fig. 4

20 Figure 4 shows the estimated values of the difference in X-ray transmission rates
21 before and after apron exchange in an experimental field. The difference in X-ray
22 transmission rates before and after apron exchange increased with the effective energy.

23

24 3-3. Practical field evaluation of X-ray protective aprons

1 In all section 2 cases, the statistical hypothesis (5) was not rejected by the F-test ($p >$
2 0.05), and the statistical hypothesis against the alternative hypothesis (6) was rejected
3 by the F-test ($p < 0.01$).

Fig. 5

4 Figure 5 shows the relationship between the exposed doses to protective aprons and
5 the transit doses through protective aprons before and after apron exchange. There were
6 no significant differences between transit doses in case a) of section 2 (Fig. 5a).
7 However, there were significant differences between transit doses in cases b) and c) of
8 section 2. In case b) of section 2 (Fig. 5c), the 0.50-mm lead-equivalent-thick non-lead
9 apron had a lower transit dose than the 0.25-mm lead apron did by 0.21 mSv per month
10 ($p < 0.01$). In case c) of section 2 (Fig. 5d), the 0.35-mm lead apron had a lower transit
11 dose than the 0.25-mm lead-equivalent-thick non-lead apron did by 0.15 mSv per month
12 ($p < 0.01$). The reductions in the annual effective dose were 2.2 mSv in case b) of
13 section 2 and 1.6 mSv in case c) of section 2.

Fig. 6

14 Figure 6 shows the t-test results for the dose reduction rates for all cases of section 2.
15 The t-test results agreed with the ANCOVA regarding all section 2 cases.

16

17

18 4. Discussion

19 There were differences between the nominal and measured lead-equivalent
20 thicknesses of protective aprons. The measured lead-equivalent thicknesses of the
21 non-lead aprons were smaller than their nominal thicknesses. This is not due to losses in
22 the lead-equivalent thicknesses of protective aprons. Because non-lead aprons include
23 low-atomic-number substances (compared with pure lead), it appears that the
24 lead-equivalent thicknesses of non-lead aprons decrease with exposure to hard radiation

1 quality caused by an additional filter, as in this study [10, 14]. Accordingly, we think
2 that the X-ray protective aprons used in this study satisfied their nominal X-ray
3 shielding performance.

4 In all section 2 cases, there were statistical differences in the X-ray transmission rates
5 before and after apron exchange. However, those evaluation did not consider the
6 difference between the experimental and practical fields. The experimental field used in
7 section 2-2-2 supposed that primary X-rays would enter at the front of the protective
8 aprons, but the practical field used in section 2-3-1 supposed that scattered X-rays
9 would enter in every direction. Consequently, two uncertainties arose regarding
10 practical field applications: the incident angle and energy of the scattered X-rays which
11 irradiate the protective apron.

12 X-ray transmission rate measurements reportedly have an uncertainty of 5% between
13 used primary and scattered X-rays [16]. In the practical field, scattered X-rays often
14 enter protective aprons in lateral and oblique directions [21]. Because IVR especially
15 makes frequent the incident angulation of the primary X-rays which irradiate the patient,
16 the uncertainty of X-ray transmission rates would exceed 5% in IVR. The X-ray
17 transmission rates depend on the X-ray energy (Fig. 3). Because scattered X-rays do not
18 always enter filters at a front angle during measurements of effective energy, the large
19 uncertainty surrounding the X-ray transmission rate arises from the measurement of the
20 scattered X-ray effective energy in the practical field. This is why applications of X-ray
21 transmission rates to practical fields appear awkward.

22 In case a) of section 2, the effective energy of the scattered X-rays would be, at most,
23 40 keV from the reference [22] regarding the X-ray energies of used apparatus.
24 Considering uncertainty beyond 5% above, the practical difference in X-ray

1 transmission rates is assumed to be a few percentage points (Fig. 4). Because the
2 exposed doses to protective aprons did not exceed 7.0 mSv per month (Fig. 5), a few
3 percentages of the X-ray transmission rate would be approximately 0.1 mSv for the
4 transit dose, which is the glass badge detection limit dose. Therefore, there was no
5 apparent significant difference in the transit doses between the non-lead aprons with
6 0.25-mm lead-equivalent thicknesses and those with 0.35-mm lead-equivalent
7 thicknesses in case a) of section 2.

8 In case b) of section 2, the effective energy of the scattered X-rays is estimated as
9 35–50 keV from the reference [23] regarding the X-ray energies of used apparatus. In
10 this effective energy range, we detected a difference of X-ray transmission rates of
11 5%–15% (Fig. 4). After apron exchange, the 0.50-mm lead-equivalent apron had a
12 marked ability to decrease the X-ray transmission rates, compared with the other aprons
13 (Fig. 3). In an experimental field, these characteristics of X-ray transmission rates
14 appear to cause significant differences in transit doses in a practical field. However, the
15 0.50-mm lead-equivalent-thick non-lead apron weighed 10.9 kg (Table 1). Orthopedic
16 spinal, hip, knee, and ankle injuries have been observed with X-ray protective aprons of
17 ≥ 5.6 kg [3]. Although the International Commission on Radiological Protection
18 publications do not provide a reference description for case b) of section 2, the National
19 Council on Radiation Protection and Measurements has advised that all new facilities
20 and practices should be designed to limit 10-mSv fractions of the annual effective doses
21 [24]. The reduction in the annual effective dose in case b) of section 2, 2.2 mSv, did not
22 exceed this 10-mSv standard. Therefore, we think that this 2.2-mSv reduction is not
23 sufficient to expose the operator to the risk of orthopedic injuries. We insist that the
24 0.25-mm lead-equivalent-thick non-lead aprons are sufficient to protect IVR operators.

1 We recommend improving some protective devices rather than wearing 0.50-mm
2 lead-equivalent non-lead aprons if additional protective measures are necessary.

3 In case c) of section 2, the effective energy of the scattered X-rays would exceed 45
4 keV from the reference [25] regarding the X-ray energies of used apparatus. With this
5 highly effective energy, we detected a difference in the X-ray transmission rates above
6 8% in an experimental field (Fig. 4). There was also a significant difference in transit
7 doses of section 3-3. Moreover, after apron exchange, the reduction in the annual
8 effective dose, 1.6 mSv, was approximately half of the annual effective dose before
9 apron exchange. However, the 0.35-mm lead-equivalent-thick lead apron after exchange
10 added 2.5 kg in weight (Table 1). We think that the risk of orthopedic injuries is small
11 because nurses in CT rooms wear X-ray protective aprons only for a few minutes while
12 acquiring CT data. We suggest that 0.35-mm lead-equivalent-thick lead aprons are
13 effective for nurses in CT rooms.

14 Finally, although the practical evaluation regarding the transit doses of protective
15 aprons involves the uncertainty about the incident angle and energy of the scattered
16 X-rays, such evaluation is convenient because effective doses as individual monitoring
17 results are usable. Moreover, the ANCOVA was as statistically precise as the t-test with
18 respect to the dose reduction rate (Fig. 6). Therefore, we propose that practical field
19 evaluations regarding the transit doses of protective aprons should be very useful for
20 feedback after apron exchange.

21 22 23 5 Conclusion

24 In this paper, we examined the effectiveness of X-ray protective aprons in 3 cases of

1 abdominal IVR, interventional cardiology, and CT. The 0.25-mm lead-equivalent-thick
2 aprons were sufficiently effective for operators in IVR because there was little
3 difference between the 0.25-mm and 0.35-mm lead-equivalent-thick aprons. The
4 0.50-mm lead-equivalent-thick non-lead apron was too heavy. The 0.35-mm lead apron
5 was effective for CT nurses because of the effectiveness against high energy X-rays
6 such as those of CT.

7 The transmission rate of protective aprons in an experimental field changes by
8 approximately 20% even in the narrow range of effective energies of 33–50 keV. When
9 X-ray protective aprons are exchanged in the future, we recommend selecting the
10 protective apron type by considering the energy of scattered X-rays in workplaces. If
11 X-ray protective aprons have already been exchanged, we recommend an additional
12 inspection regarding their effectiveness in the practical field, because the result will not
13 always agree with those of experimental field evaluations.

14

15

16 Acknowledgments

17 This study was supported in part by the Hokkaido Radiological Technology Study
18 from the Hokkaido meeting of the Japanese Society of Radiological Technology in 2010.
19 The manuscript was partly supported by Akiyoshi Ohtsuka Fellowship of the Japanese
20 Society of Radiological Technology for improvement in English expression of a draft
21 version of the manuscript. A portion of this paper was presented at the 96th Scientific
22 Assembly and Annual Meeting of the Radiological Society of North America in 2010 by
23 an international workshop delegate of the Japanese Society of Radiological Technology.

24

1

2 Conflict of Interest

3 The authors have no conflicts of interest in connection with this paper.

4

1 References

- 2 1. Klein LW, Miller DL, Balter S, Laskey W, Haines D, Norbash A, Mauro MA,
3 Goldstein JA. Occupational health hazards in the interventional laboratory: time for
4 a safer environment. *Radiology*. 2009;250:538-44.
- 5 2. Moore B, vanSonnenberg E, Casola G, Novelline RA. The relationship between
6 back pain and lead apron use in radiologists. *Am J Roentgenol*. 1992;158:191-3.
- 7 3. Ross AM, Segal J, Borenstein D, Jenkins E, Cho S. Prevalence of spinal disk disease
8 among interventional cardiologists. *Am J Cardiol*. 1997;79:68-70.
- 9 4. Webster EW. Experiments with medium Z-materials for shielding against
10 low-energy x-rays. *Radiology*. 1966;86:146.
- 11 5. Webster EW. Addendum to 'Composite materials for x-ray protection'. *Health Phys*.
12 1991;61:917-8.
- 13 6. Zuguchi M, Chida K, Taura M, Inaba Y, Ebata A, Yamada S. Usefulness of non-lead
14 aprons in radiation protection for physicians performing interventional procedures.
15 *Radiat Prot Dosimetry*. 2008;131:531-4.
- 16 7. Yaffe MJ, Mawdsley GE, Lilley M, Servant R, Reh G. Composite materials for
17 x-ray protection. *Health Phys*. 1991;60:661-4.
- 18 8. Murphy PH, Wu Y, Glaze SA. Attenuation properties of lead composite aprons.
19 *Radiology*. 1993;186:269-72.
- 20 9. Takano Y, Okazaki K, Ono K, Kai M. Experimental and theoretical studies on
21 radiation protective effect of a lighter non-lead protective apron. *Nihon Hoshasen*
22 *Gijutsu Gakkai Zasshi*. 2005;61:1027-32. (in Japanese)
- 23 10. Kumagai M, Shintani M, Kuranishi M. Evaluation of X-ray shielding performance
24 of protective aprons. *Nihon Hoshasen Gijutsu Gakkai Zasshi*. 1999;55:379-84. (in

- 1 Japanese)
- 2 11. Christodoulou EG, Goodsitt MM, Larson SC, Darner KL, Satti J, Chan HP.
3 Evaluation of the transmitted exposure through lead equivalent aprons used in a
4 radiology department, including the contribution from backscatter. *Med Phys.*
5 2003;30:1033-8.
- 6 12. JCS Joint Working Group. Guidelines for radiation safety in interventional
7 cardiology (JCS 2006). *Circ J.* 2006;70:1278-80. (in Japanese)
- 8 13. Awai K. Study reports in radiation exposure for a medical workers and protective
9 clothing in recent X-ray study. *Nihon Hoshasen Gijutsu Gakkai Zasshi.*
10 1998;54:687-96. (in Japanese)
- 11 14. Inoue S, Matsumoto M, Matsuzawa R. Examination of optimal radiation quality in
12 the lead equivalent examination of X-ray protective clothing. *Nihon Hoshasen*
13 *Gijutsu Gakkai Zasshi.* 2004;60:1682-7. (in Japanese)
- 14 15. Seltzer SM, Hubbell J. Tables and graphs of photon mass attenuation coefficients
15 and mass energy-absorption coefficients for photon energies 1 keV to 20 MeV for
16 elements $Z=1$ to 92 and some dosimetric materials. Kyoto: Japanese society of
17 radiological technology; 1995. (in Japanese)
- 18 16. Rawlings DJ, Faulkner K, Harrison RM. Broad-beam transmission data in lead for
19 scattered radiation produced at diagnostic energies. *Br J Radiol.* 1991;64:69-71.
- 20 17. Albert RW, Olli TA. Analysis of covariance. London: Sage Publications, Inc.; 1978,
21 p. 7-54.
- 22 18. Armitage P, Berry G, Matthews JNS. Statistical methods in medical research.
23 Massachusetts: Wiley-Blackwell, Inc.; 2001, p. 331-7.
- 24 19. International Commission on Radiation Units and Measurements (ICRU). Quantities

- 1 and units in radiation protection dosimetry: ICRU Report. 1993; p. 51.
- 2 20. Nuclear Safety Technology Center. Hibakusenryou-no-sokutei/hyouka-manyuaru.
3 Tokyo: 2000, p. 45-7. (in Japanese)
- 4 21. Iida H, Chabatake M, Shimizu M, Tamura S. Radiation Protection of Angiographers
5 in Interventional Radiology. Nihon Hoshasen Gijutsu Gakkai Zasshi.
6 2001;57:1548-55. (in Japanese)
- 7 22. Mori H, Koshida K, Ichikawa K. Estimation of personal dose based on the
8 dependent calibration of personal dosimeters in interventional radiology. Nihon
9 Hoshasen Gijutsu Gakkai Zasshi. 2007;63:852-61. (in Japanese)
- 10 23. Fukuda A, Koshida K, Yamaguchi I, Togashi A, Matsubara K. Method of estimating
11 patient skin dose from dose displayed on medical X-ray equipment with flat panel
12 detector. Nihon Hoshasen Gijutsu Gakkai Zasshi. 2004;60:725-33. (in Japanese)
- 13 24. National Council on Radiation Protection and Measurements (NCRP). Limitation of
14 exposure to ionizing radiation: NCRP report. 1993;116:33-5.
- 15 25. Iida H, Noto K, Mitsui W, Takata T, Yamamoto T, Matsubara K. New method of
16 measuring effective energy using copper-pipe absorbers in X-ray CT. Nihon
17 Hoshasen Gijutsu Gakkai Zasshi. 2011;67:1183-91. (in Japanese)

18

1 Fig. 1 Geometry of an experimental field for measuring the lead-equivalent
2 thicknesses and X-ray transmission rates of protective aprons.

3 Fig. 2 Relationship between the tube potential and the effective energy of the primary
4 X-rays in an experimental field.

5 Fig. 3 Relationship between effective energy and X-ray transmission rates of
6 protective aprons in an experimental field. '[]' in figures expresses the
7 lead-equivalent thicknesses of X-ray protective aprons. (a-1) Comparison of
8 protective apron types before and after exchange for the first abdominal
9 interventional radiology operator. (a-2) Comparison of protective apron types
10 before and after exchange for the second abdominal interventional radiology
11 operator. (b) Comparison of protective apron types before and after exchange for
12 the interventional cardiology operator. (c) Comparison of protective apron types
13 before and after exchange for computed tomography nurses.

14 Fig. 4 Difference in X-ray transmission rates before and after apron exchange in an
15 experimental field. Cases a), b), and c) upon exchange of the protective apron type
16 are described at the beginning of section 2.

17 Fig. 5 Relationship between the exposed doses to protective aprons
18 ($H_P(10)_{\text{collar/month}}$) and the transmitted doses through protective aprons
19 ($H_P(10)_{\text{body/month}}$) before and after the apron exchange in a practical field. These
20 occupational doses express the personal dose equivalents, which are defined by
21 International Commission on Radiation Units and Measurements (ICRU) Report 51
22 [19] in tissues at a depth of 10 mm. '[]' and ' $|\alpha_2 - \alpha_1|_{95\%}$ ' in figures express
23 the lead-equivalent thicknesses of the X-ray protective aprons and the 95%

1 confidence interval, respectively. (a-1) Comparison between 0.25-mm and 0.35-mm
2 lead-equivalent-thick non-lead aprons as worn by the first abdominal interventional
3 radiology operator. (a-2) Comparison between 0.25-mm and 0.35-mm
4 lead-equivalent-thick non-lead aprons as worn by the second abdominal
5 interventional radiology operator. (b) Comparison between 0.25-mm lead apron and
6 0.50-mm lead-equivalent-thick non-lead apron as worn by the interventional
7 cardiology operator. (c) Comparison between 0.25-mm lead-equivalent-thick
8 non-lead apron and 0.35-mm lead apron as worn by computed tomography nurses.

9 Fig. 6 Difference in the dose reduction rate before and after the exchange of
10 protective apron types in a practical field. '[]' in a figure expresses the
11 lead-equivalent thicknesses of the X-ray protective aprons.

12 Table 1 Specifications and use conditions of the X-ray protective aprons. The upper and
13 lower aprons for each case are the types of protective aprons used before and after
14 the exchange.

15 Table 2 Nominal and measured lead-equivalent thicknesses of the X-ray protective
16 aprons. The upper and lower aprons for each case are the types of protective aprons
17 used before and after the exchange.

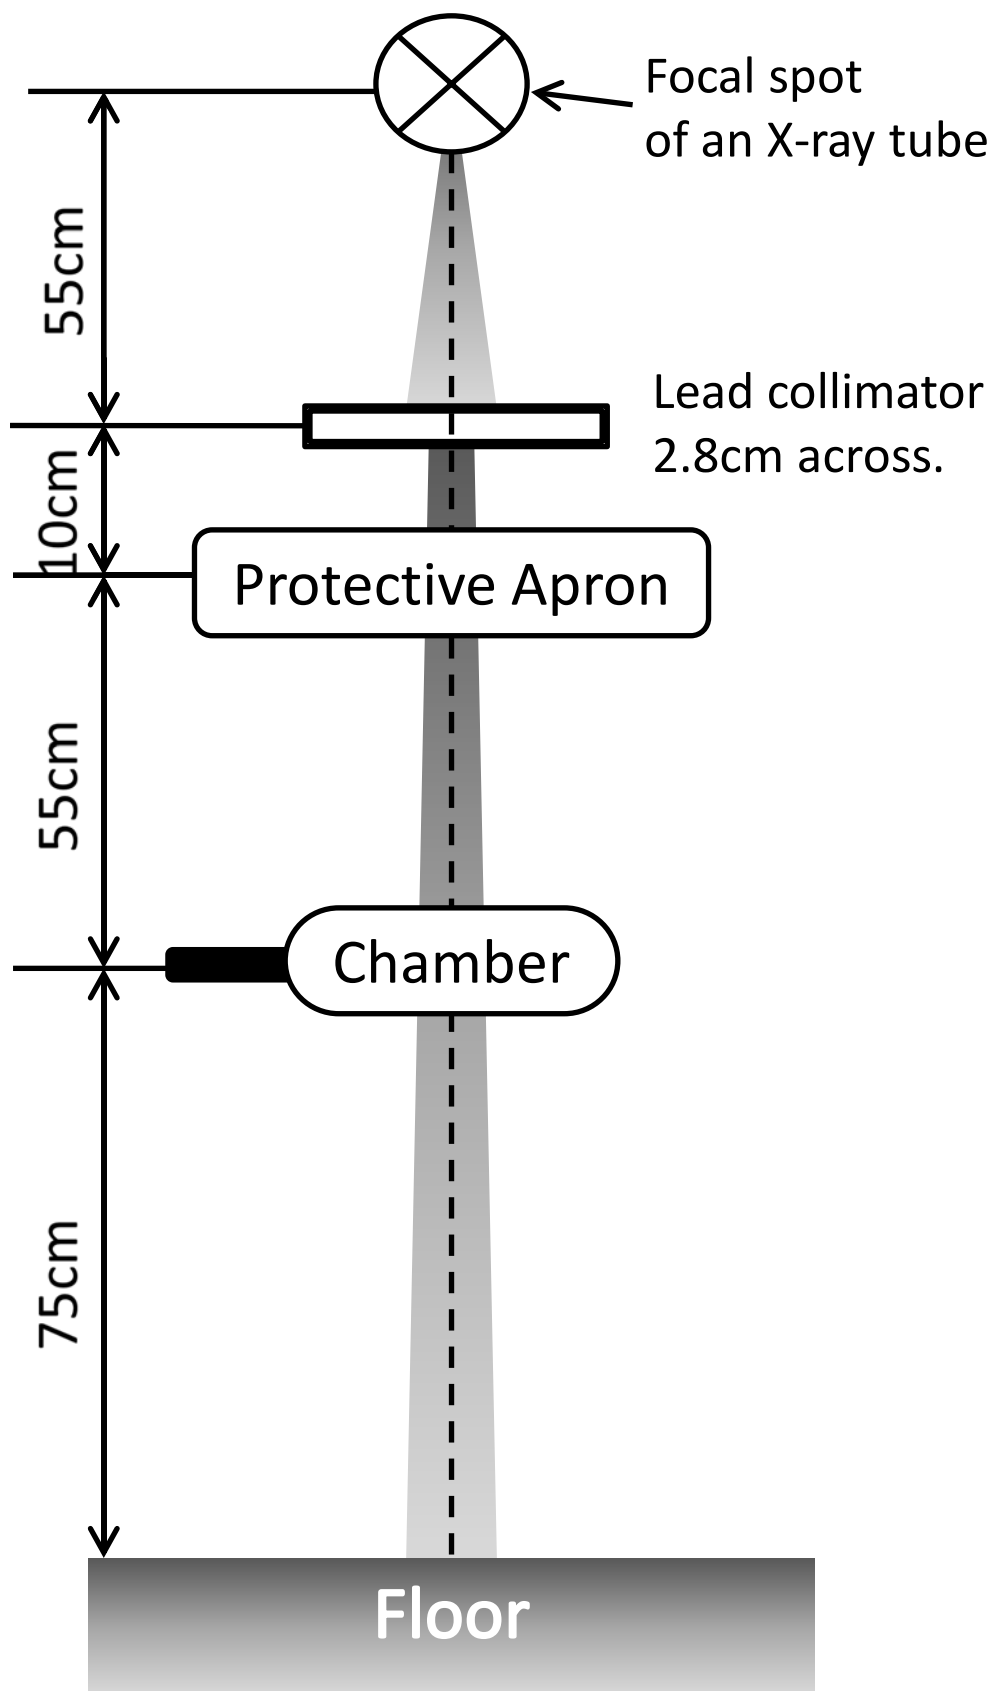


Fig. 1 Geometry of an experimental field for measuring the lead-equivalent thicknesses and X-ray transmission rates of protective aprons.

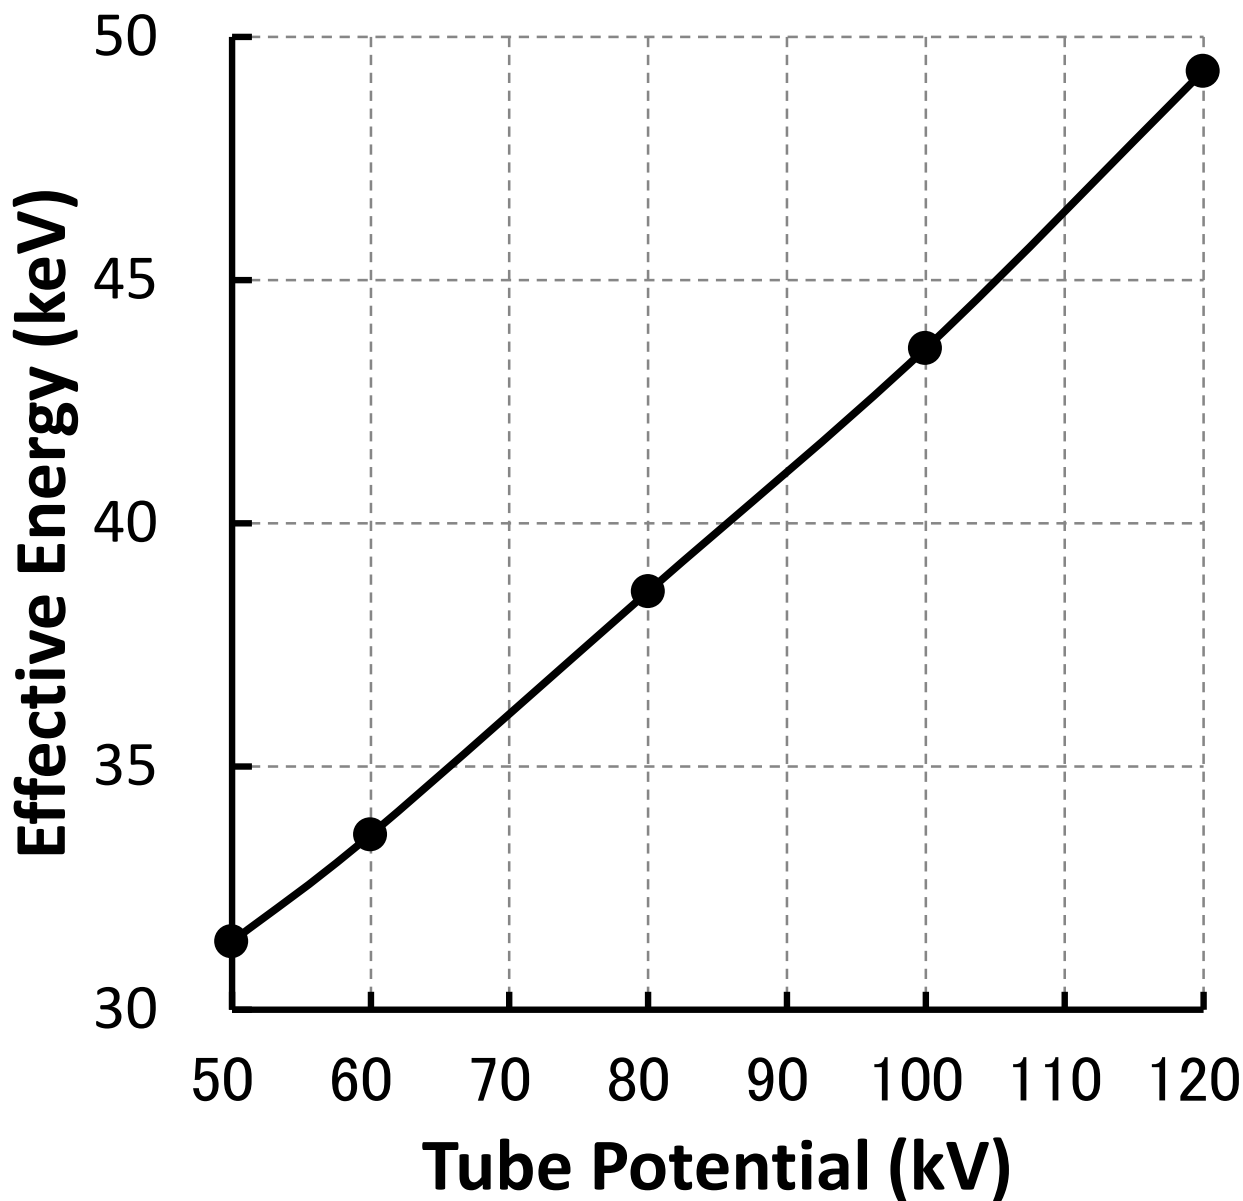


Fig. 2 Relationship between the tube potential and the effective energy of the primary X-rays in an experimental field.

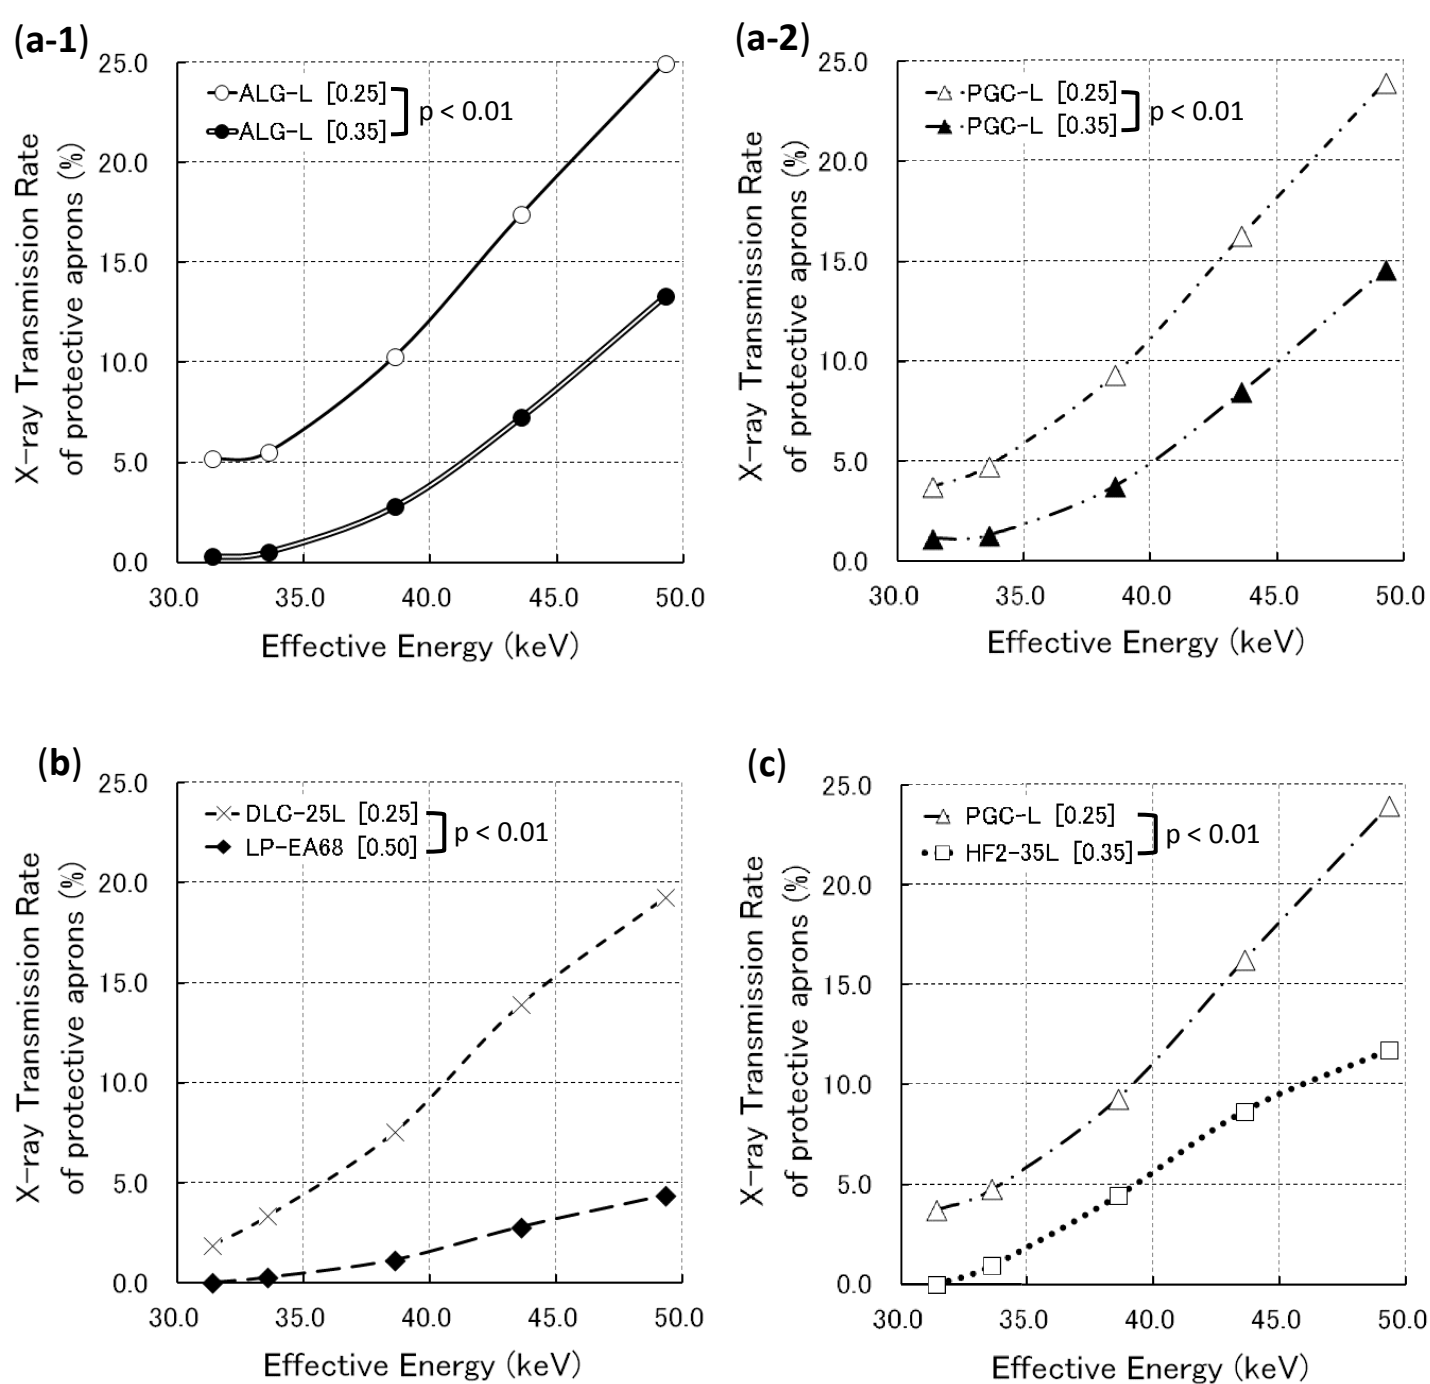


Fig. 3 Relationship between effective energy and X-ray transmission rates of protective aprons in an experimental field. ‘[]’ in figures expresses the lead-equivalent thicknesses of X-ray protective aprons. **(a-1)** Comparison of protective apron types before and after exchange for the first abdominal interventional radiology operator. **(a-2)** Comparison of protective apron types before and after exchange for the second abdominal interventional radiology operator. **(b)** Comparison of protective apron types before and after exchange for the interventional cardiology operator. **(c)** Comparison of protective apron types before and after exchange for computed tomography nurses.

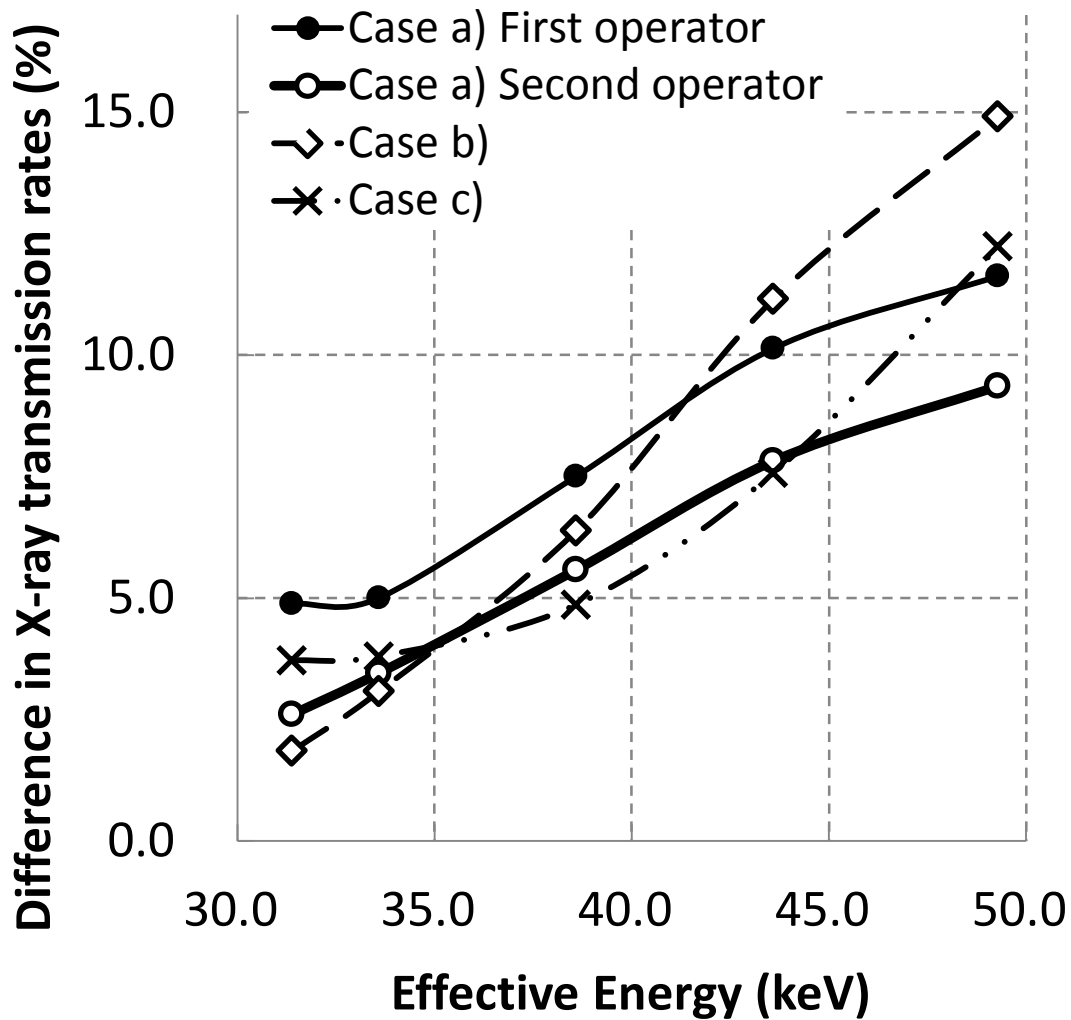


Fig. 4 Difference in X-ray transmission rates before and after apron exchange in an experimental field. Cases a), b), and c) upon exchange of the protective apron type are described at the beginning of section 2.

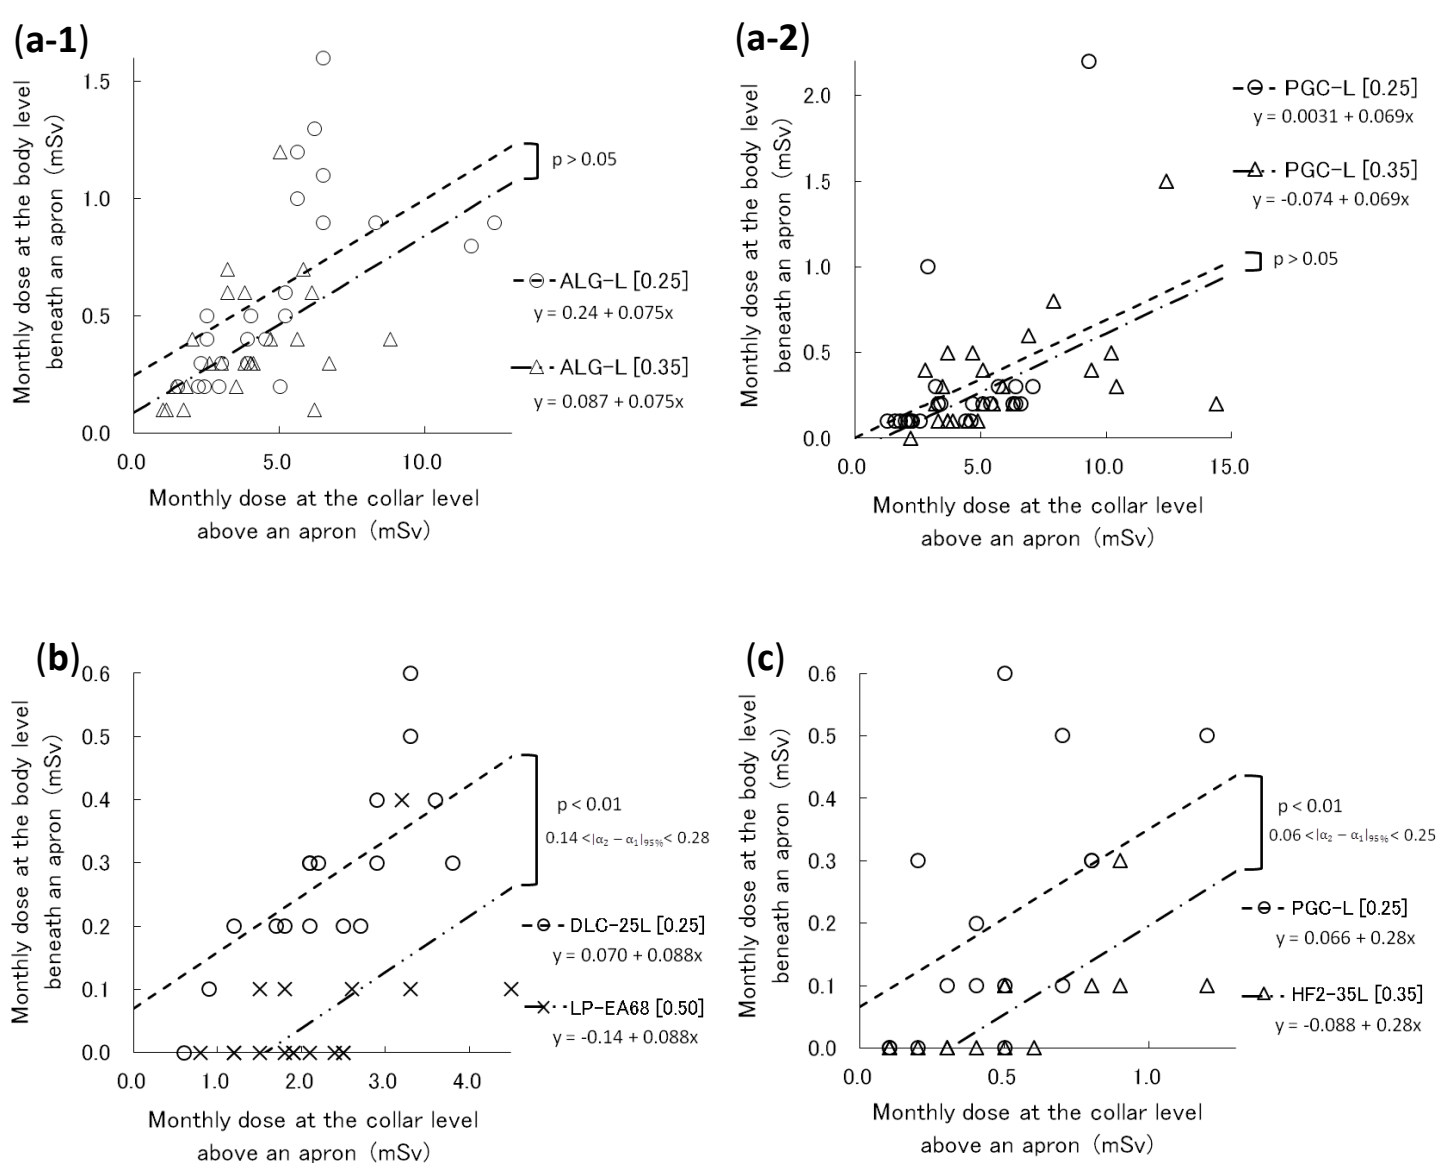


Fig. 5 Relationship between the exposed doses to protective aprons ($H_P(10)_{\text{collar}}/\text{month}$) and the transmitted doses through protective aprons ($H_P(10)_{\text{body}}/\text{month}$) before and after the apron exchange in a practical field. These occupational doses express the personal dose equivalents, which are defined by International Commission on Radiation Units and Measurements (ICRU) Report 51 [19] in tissues at a depth of 10 mm. ‘ [] ’ and ‘ $|\alpha_2 - \alpha_1|_{95\%}$ ’ in figures express the lead-equivalent thicknesses of the X-ray protective aprons and the 95% confidence interval, respectively. **(a-1)** Comparison between 0.25-mm and 0.35-mm lead-equivalent-thick non-lead aprons as worn by the first abdominal interventional radiology operator. **(a-2)** Comparison between 0.25-mm and 0.35-mm lead-equivalent-thick non-lead aprons as worn by the second abdominal interventional radiology operator. **(b)** Comparison between 0.25-mm lead apron and 0.50-mm lead-equivalent-thick non-lead apron as worn by the interventional cardiology operator. **(c)** Comparison between 0.25-mm lead-equivalent-thick non-lead apron and 0.35-mm lead apron as worn by computed tomography nurses.

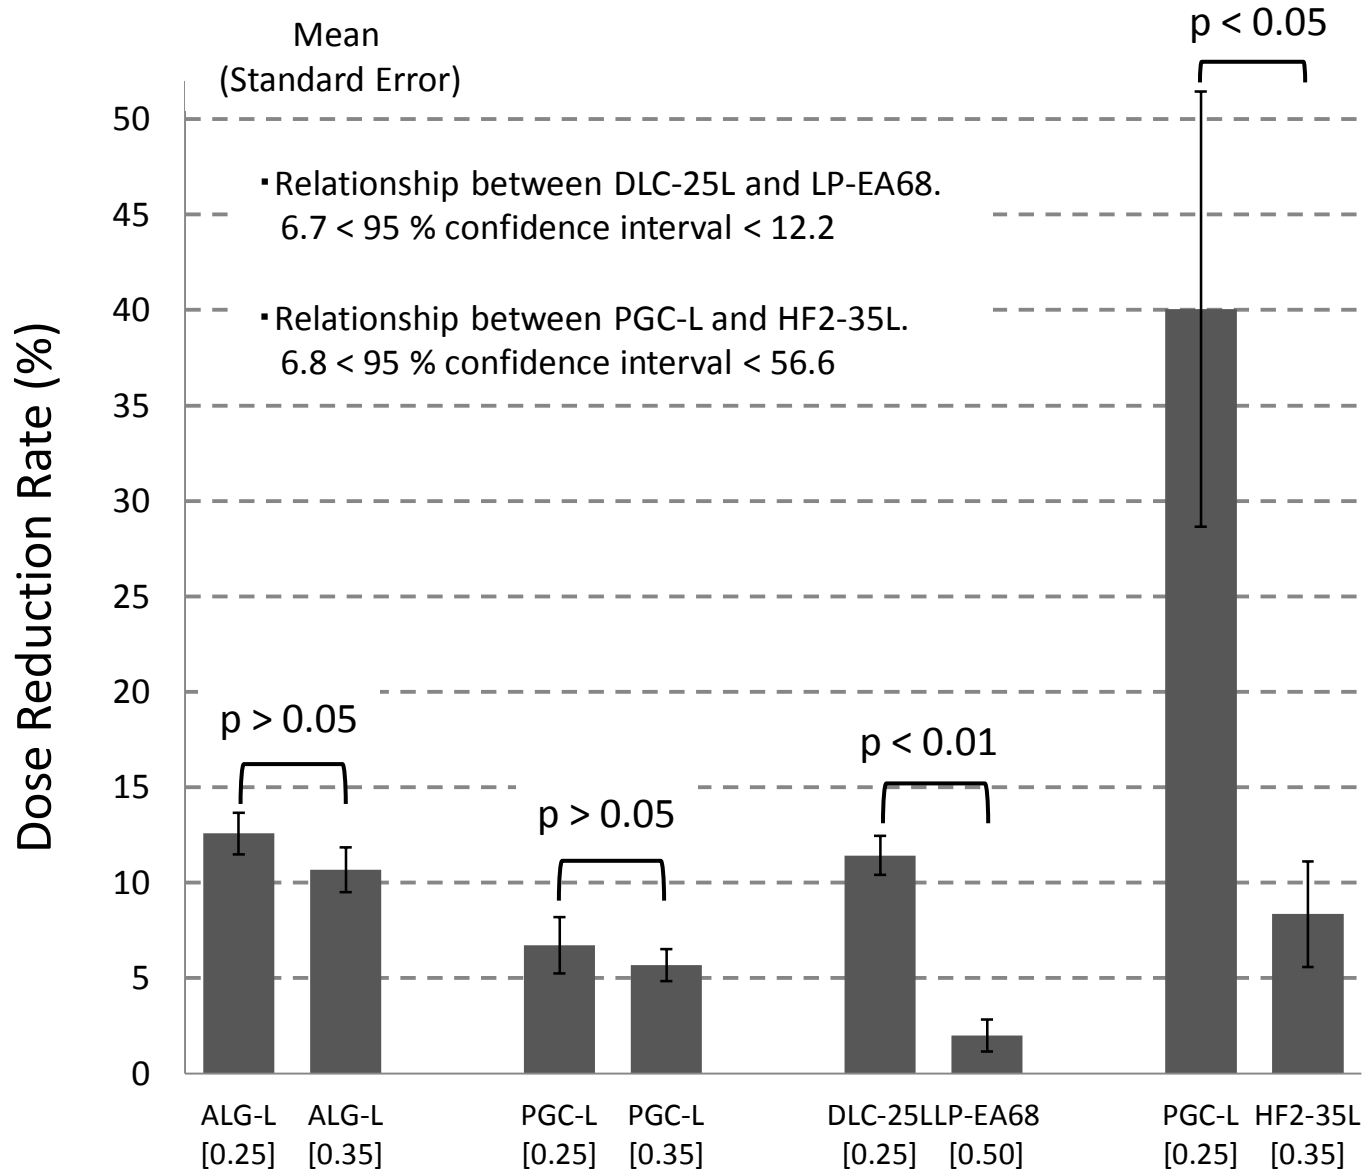


Fig. 6 Difference in the dose reduction rate before and after the exchange of protective apron types in a practical field. ‘[]’ in a figure expresses the lead-equivalent thicknesses of the X-ray protective aprons.

Table 1 Specifications and use conditions of the X-ray protective aprons. The upper and lower aprons for each case are the types of protective aprons used before and after the exchange.

Model	Maker	Weight	Lead		Medical X-ray Apparatus Used in Workplaces
			Lead or not ^{*1}	Nominal Thickness ^{*2}	
Case a) Abdominal Interventional Radiology Operators					
<i>First Operator</i>					
ALG-L	Hoshina	2.7 kg	(-)	0.25 mm	Infinix Celeve VC
ALG-L	Hoshina	3.6 kg	(-)	0.35 mm	Toshiba Medical Systems
<i>Second Operator</i>					
PGC-L	Hoshina	2.9 kg	(-)	0.25 mm	Infinix Celeve VC
PGC-L	Hoshina	3.8 kg	(-)	0.35 mm	Toshiba Medical Systems
Case b) Interventional Cardiology Operator					
DLC-25L	Maeda	3.6 kg	(+)	0.25 mm	INNOVA 2000
LP-EA68	AADCO Medical	10.9 kg	(-)	0.50 mm	GE Healthcare Japan
Case c) Computed Tomography Nurses					
PGC-L	Hoshina	2.9 kg	(-)	0.25 mm	LightSpeed VCT scanner with
HF2-35L	Maeda	5.4 kg	(+)	0.35 mm	62 rows of detector elements GE Healthcare Japan

Hoshina, Maeda, and GE Healthcare Japan: Tokyo, Japan.

AADCO Medical: Rondolph Vermont, USA. Toshiba Medical Systems: Tochigi, Japan.

*1 'Lead or not' expresses whether an X-ray protective apron involves lead '(+)', or not '(-)'.

*2 'Nominal Thickness' expresses the nominal lead-equivalent thickness of an X-ray protective apron.

Table 2 Nominal and measured lead-equivalent thicknesses of the X-ray protective aprons. The upper and lower aprons for each case are the types of protective aprons used before and after the exchange.

Model	Lead-equivalent Thickness of protective aprons	
	Nominal Value	Measured Value
Case a) Abdominal Interventional Radiology Operators		
<i>First Operator</i>		
ALG-L	0.25 mm	0.20 mm
ALG-L	0.35 mm	0.31 mm
<i>Second Operator</i>		
PGC-L	0.25 mm	0.21 mm
PGC-L	0.35 mm	0.29 mm
Case b) Interventional Cardiology Operator		
DLC-25L	0.25 mm	0.25 mm*
LP-EA68	0.50 mm	0.52 mm [#]
Case c) Computed Tomography Nurses		
PGC-L	0.25 mm	0.21 mm
HF2-35L	0.35 mm	0.34 mm*

* expresses X-ray protective apron involving lead.

[#] is the measured value with an additional shield.